



# DEL MEDICAL SYSTEMS GROUP

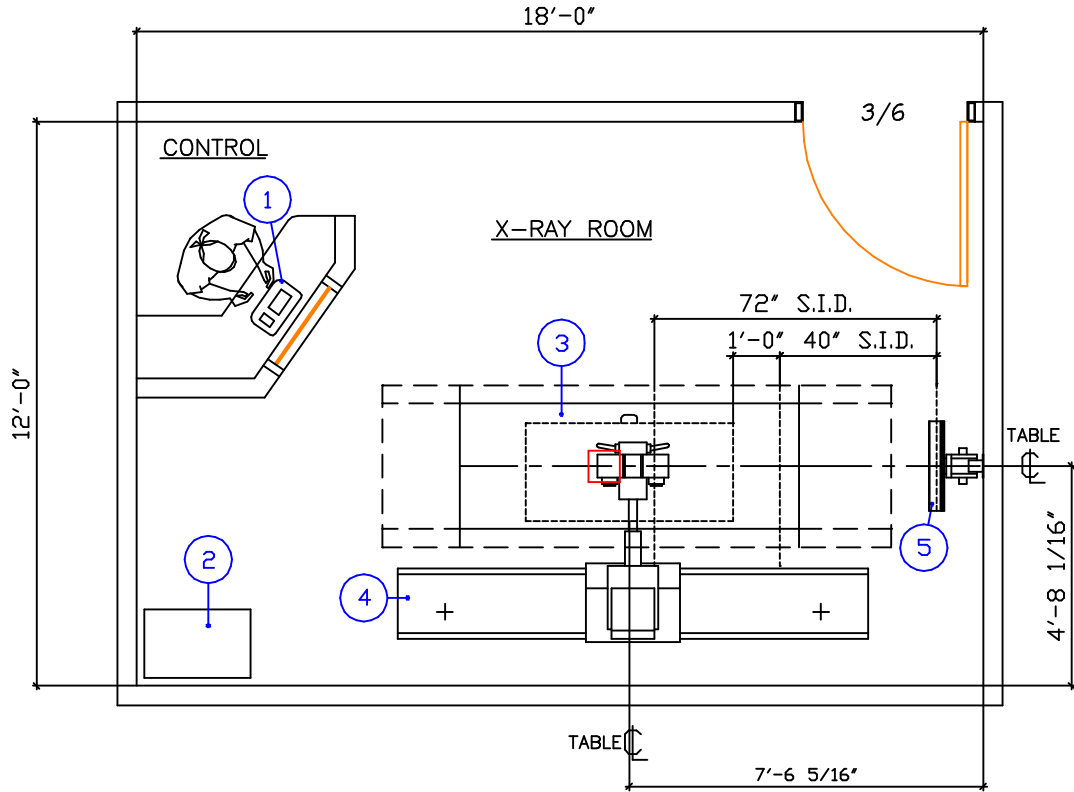

## GENERAL NOTES

- ALL SPECIFICATIONS AND SPACE REQUIREMENTS ARE SHOWN GENERICALLY. CONTACT GAMMA TECH, INC. FOR SPECIFIC REQUIREMENTS PERTAINING TO OPTIONAL EQUIPMENT COMPONENTS AND SITE SPECIFIC ROOM PLANNING.
- RECOMMENDED CEILING HEIGHT IS 8'-0".
- SUGGESTED AMBIENT ROOM REQUIREMENTS ARE 66° TO 75° F. AT 30% TO 60% R.M. (NON-CONDENSING).
- MAIN INCOMING POWER SUPPLY: VARIES WITH GENERATOR KW MODEL.

## EQUIPMENT SCHEDULE

| NO. | EQUIPMENT IDENTIFICATION NUMBER |   |               |       |        |     |
|-----|---------------------------------|---|---------------|-------|--------|-----|
|     | BTU / HOUR                      | DESCRIPTION   | WEIGHT (LBS.) |       |        |     |
|     |                                 |   | W             | D     | H      |     |
| 1   | 320                             | DEL MEDICAL SYSTEMS GROUP<br>APX SERIES HF GENERATOR<br>OPERATOR CONTROL PANEL          | 13.25         | 7.86  | VARIES | 25  |
| 2   | 4000                            | DEL MEDICAL SYSTEMS GROUP<br>APX SERIES HF GENERATOR<br>RACK CABINET                    | 27.00         | 17.50 | 45.75  | 300 |
| 3   | 300                             | DEL MEDICAL SYSTEMS GROUP<br>EV-650<br>ELEVATING 4-WAY FLOAT TOP TABLE                  | 86.62         | 31.90 | 33.70  | 585 |
| 4   | 1200                            | DEL MEDICAL SYSTEMS GROUP<br>MODEL DFMT/FMFS (TRUNION MOUNT)<br>FLOOR MOUNTED TUBESTAND | 120.00        | 45.00 | 85.00  | 673 |
| 5   | 35                              | DEL MEDICAL SYSTEMS GROUP<br>3546<br>14' X 17' WALLSTAND                                | 23.00         | 14.00 | 86.00  | 250 |
| 6   |                                 |   |               |       |        |     |
| 7   |                                 |   |               |       |        |     |
| 8   |                                 |   |               |       |        |     |

## TYPICAL M1A SYSTEM HIGH FREQUENCY RADIOGRAPHIC SUITE



**GAMMA TECH, INC.**

1213 Idaho Road  
Austintown, OH 44515  
dhenry@gammatech.net

Voice (330) 792-9568  
Fax (330) 792-0658  
www.gammatech.net

DESIGNER:  
**DAVID HENRY**

FILE NAME: DEL3TYP.DWG  
REVISION DATE: 05/28/2008