




# GE Medical Systems

## GE HISPEED ZXi CT SCANNER

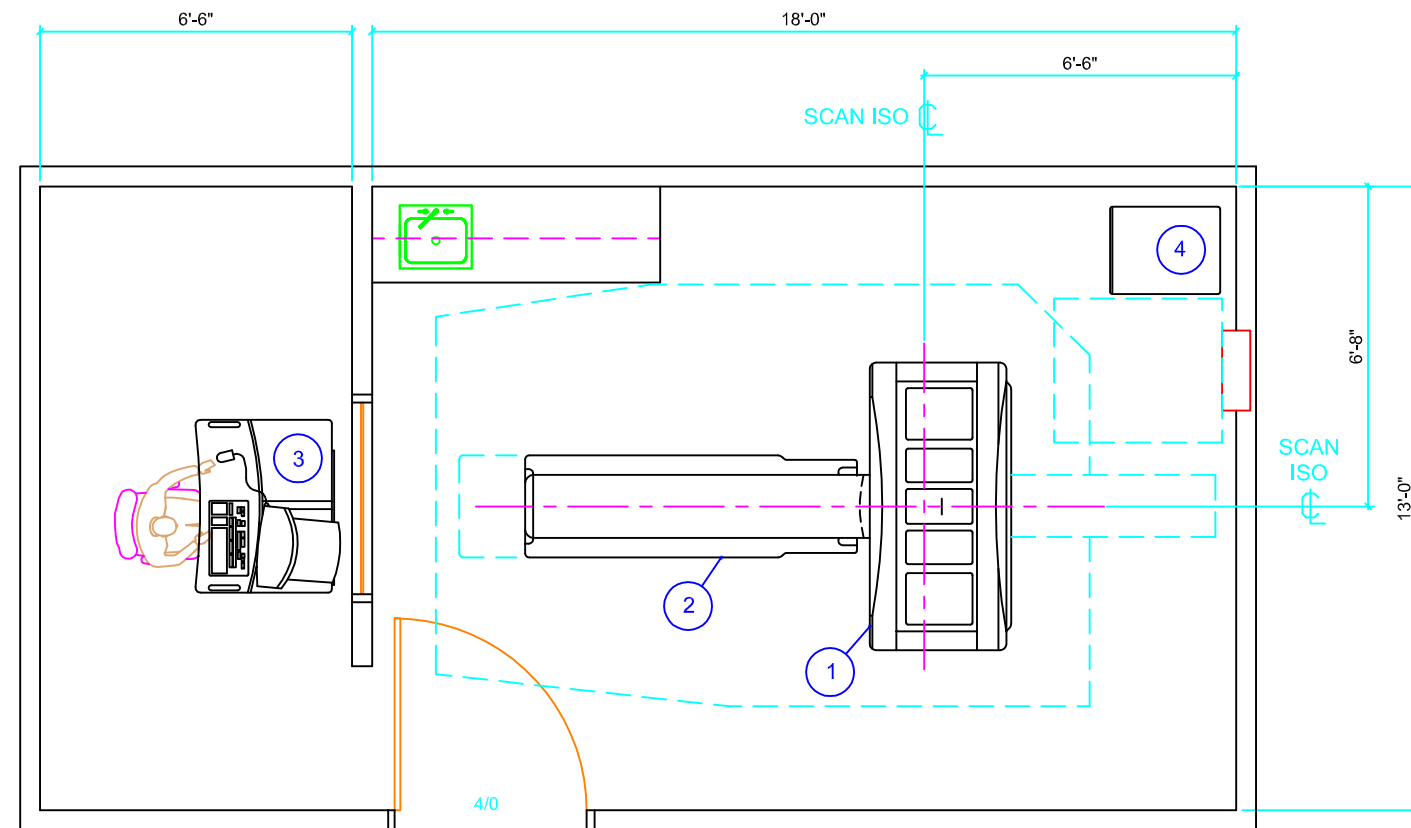

**TYPICAL ROOM AND EQUIPMENT LAYOUT**  
(DASHED LINES DEPICT EQUIPMENT TRAVEL AND SERVICE CLEARANCES)  
RECOMMENDED FINISHED CEILING HEIGHT IS 9'-0"

### GENERAL NOTES

- ALL SPECIFICATIONS AND SPACE REQUIREMENTS ARE SHOWN GENERICALLY. CONTACT GAMMA TECH, INC. FOR SPECIFIC REQUIREMENTS PERTAINING TO OPTIONAL EQUIPMENT COMPONENTS AND ADDITIONAL ROOM PREPARATION SPECIFICATIONS.
- RECOMMENDED FINISHED CEILING HEIGHT IS 9'-0".  
MINIMUM FINISHED CEILING HEIGHT IS 7'-6".
- AMBIENT OPERATION TEMPERATURE: 68° TO 82° F.  
HUMIDITY: 30% TO 70% (NON-CONDENSING).  
ALLOWABLE TEMPERATURE CHANGE: 8°F PER HOUR  
ALLOWABLE HUMIDITY CHANGE: 5% PER HOUR  
MAX - ALTITUDE: 8,200FT ABOVE SEA LEVEL
- MAIN INCOMING POWER SUPPLY:  
480VAC, THREE PHASE, 112.5KVA, DELTA OR WYE, 90AMP, 3 POLE, MAIN CB  
5% VOLTAGE REGULATION, 90% POWER FACTOR

© PLANNING DIVISION

FILE NAME:  
GE HISPEED ZXI

REVISION DATE:  
07.02.2008

### EQUIPMENT SCHEDULE

#### EQUIPMENT IDENTIFICATION NUMBER

EQUIPMENT IDENTIFICATION NUMBER	BTU / HOUR	DESCRIPTION	WEIGHT (LBS.)			
			DIMENSIONS (IN.)			
			W	x	D	x
1	16260	GENERAL ELECTRIC MEDICAL SYSTEMS HISPEED ZXi GANTRY	71.65	35.32	72.84	2580
2	318	GENERAL ELECTRIC MEDICAL SYSTEMS HISPEED ZXi PATIENT TABLE WITHOUT EXTENDED TABLE TOP	25.60	88.32	37.40	651
3	2911	GENERAL ELECTRIC MEDICAL SYSTEMS HISPEED ZXi OPERATOR'S CONSOLE / COMPUTER	43.31	33.90	51.90	449
4	615	GENERAL ELECTRIC MEDICAL SYSTEMS HISPEED ZXi POWER DISTRIBUTION UNIT	21.66	27.56	32.29	346

PLANNING BY:



**GAMMA TECH, INC**

129 Wild Berry Lane  
Hampstead, NC 28443  
Ph (910) 270-9787 • Fax (910) 270-9767  
www.gammatech.net

