




GE Medical Systems

GE LIGHTSPEED QXi CT SCANNER

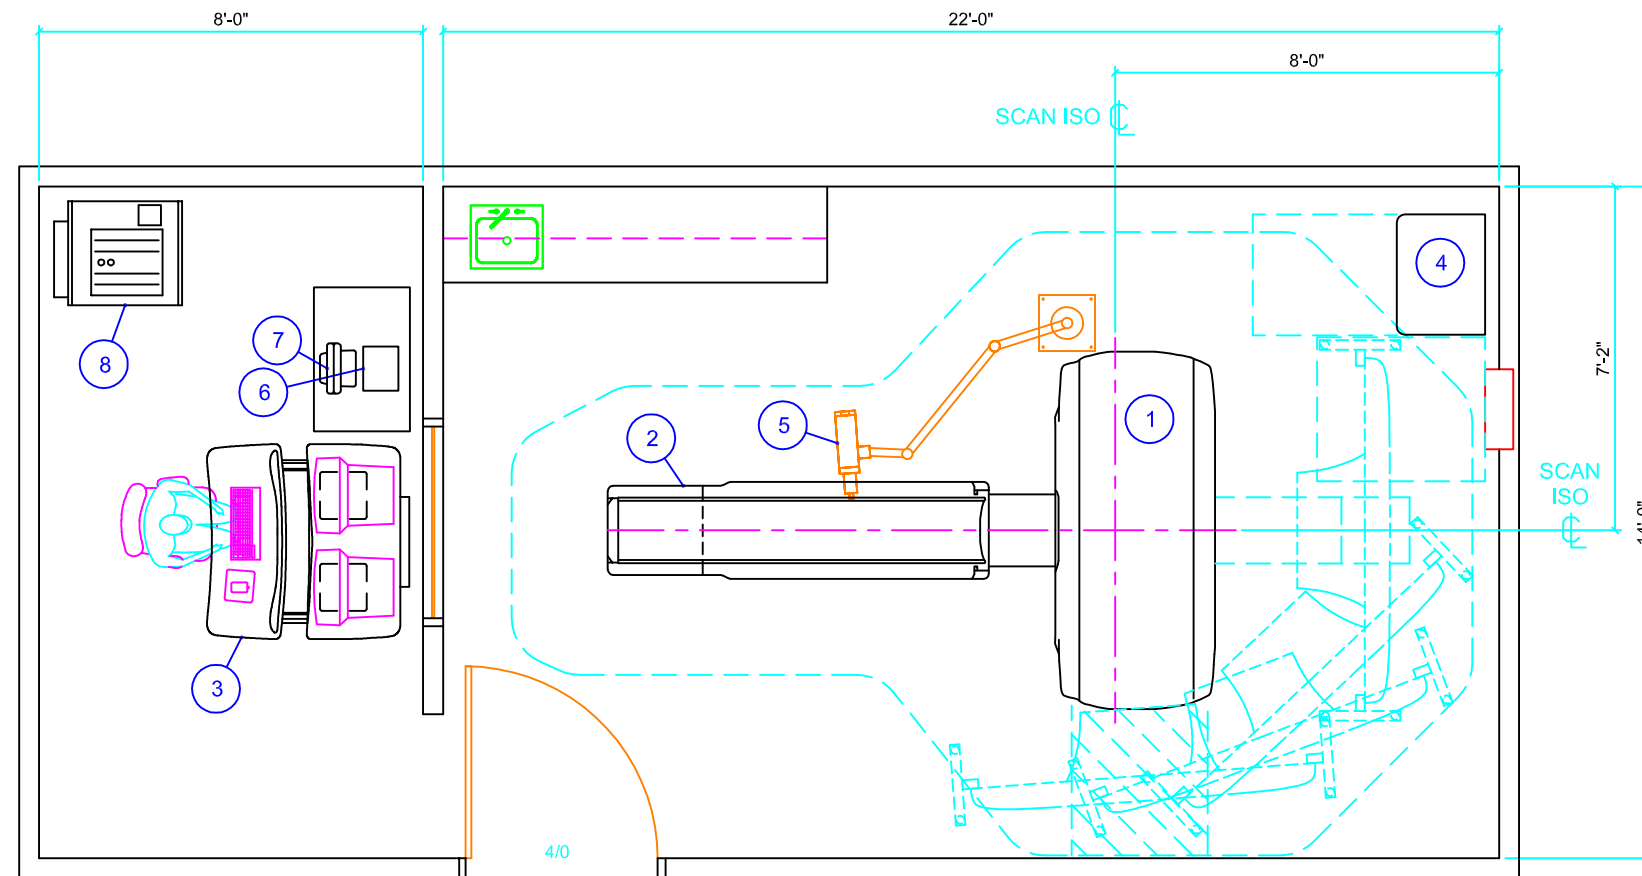

TYPICAL ROOM AND EQUIPMENT LAYOUT
(DASHED LINES DEPICT EQUIPMENT TRAVEL AND SERVICE CLEARANCES)
RECOMMENDED FINISHED CEILING HEIGHT IS 9'-0"

GENERAL NOTES

- ALL SPECIFICATIONS AND SPACE REQUIREMENTS ARE SHOWN GENERICALLY. CONTACT GAMMA TECH, INC. FOR SPECIFIC REQUIREMENTS PERTAINING TO OPTIONAL EQUIPMENT COMPONENTS AND ADDITIONAL ROOM PREPARATION SPECIFICATIONS.
- RECOMMENDED FINISHED CEILING HEIGHT IS 9'-0".
MINIMUM FINISHED CEILING HEIGHT IS 7'-8".
- AMBIENT OPERATION TEMPERATURE: 60° TO 75° F.
HUMIDITY: 30% TO 60% (NON-CONDENSING).
ALLOWABLE TEMPERATURE CHANGE: 5°F PER HOUR
ALLOWABLE HUMIDITY CHANGE: 5% PER HOUR
MAX - ALTITUDE: 10,000FT ABOVE SEA LEVEL
- MAIN INCOMING POWER SUPPLY:
480VAC, THREE PHASE, 112.5KVA, DELTA OR WYE, 90AMP, 3 POLE, MAIN CB
5% VOLTAGE REGULATION, 85% POWER FACTOR

© PLANNING DIVISION

FILE NAME:
GE LIGHTSPEED QXi

REVISION DATE:
01.31.2008

EQUIPMENT SCHEDULE

EQUIPMENT IDENTIFICATION NUMBER

EQUIPMENT IDENTIFICATION NUMBER	BTU / HOUR	DESCRIPTION	WEIGHT (LBS.)			
			DIMENSIONS (IN.)			
			W	x	D	x
1	24403	GENERAL ELECTRIC MEDICAL SYSTEMS LIGHTSPEED QXi CT SCANNER GANTRY	86.60	39.24	74.62	3120
2	700	GENERAL ELECTRIC MEDICAL SYSTEMS LIGHTSPEED QXi CT SCANNER PATIENT TABLE WITH EXTENDED TABLE TOP	24.00	94.91	41.71	1185
3	12481	GENERAL ELECTRIC MEDICAL SYSTEMS LIGHTSPEED QXi CT SCANNER OPERATOR'S CONSOLE / COMPUTER	48.73	48.35	34.76	608
4	3412	GENERAL ELECTRIC MEDICAL SYSTEMS LIGHTSPEED QXi CT SCANNER POWER DISTRIBUTION UNIT	30.00	22.00	50.00	800
5	N/A	MEDRAD STELLANT CT INJECTOR SYSTEM HEAD ON CEILING MOUNT COUNTERPOISE				
6	N/A	MEDRAD STELLANT CT INJECTOR SYSTEM ELECTRONICS BASE UNIT (ON DESK)	11.00	8.80	11.50	14
7	N/A	MEDRAD STELLANT CT INJECTOR SYSTEM DISPLAY CONTROL CONSOLE (ON DESK)	12.50	8.90	13.50	8
8	2300	KODAK DRYVIEW 8700 LASER IMAGER	26.02	32.00	50.35	550

PLANNING BY:



GAMMA TECH, INC

129 Wild Berry Lane
Hampstead, NC 28443
Ph (910) 270-9787 • Fax (910) 270-9767
www.gammatech.net

