




# GE Medical Systems

## CT PACE CT SCANNER

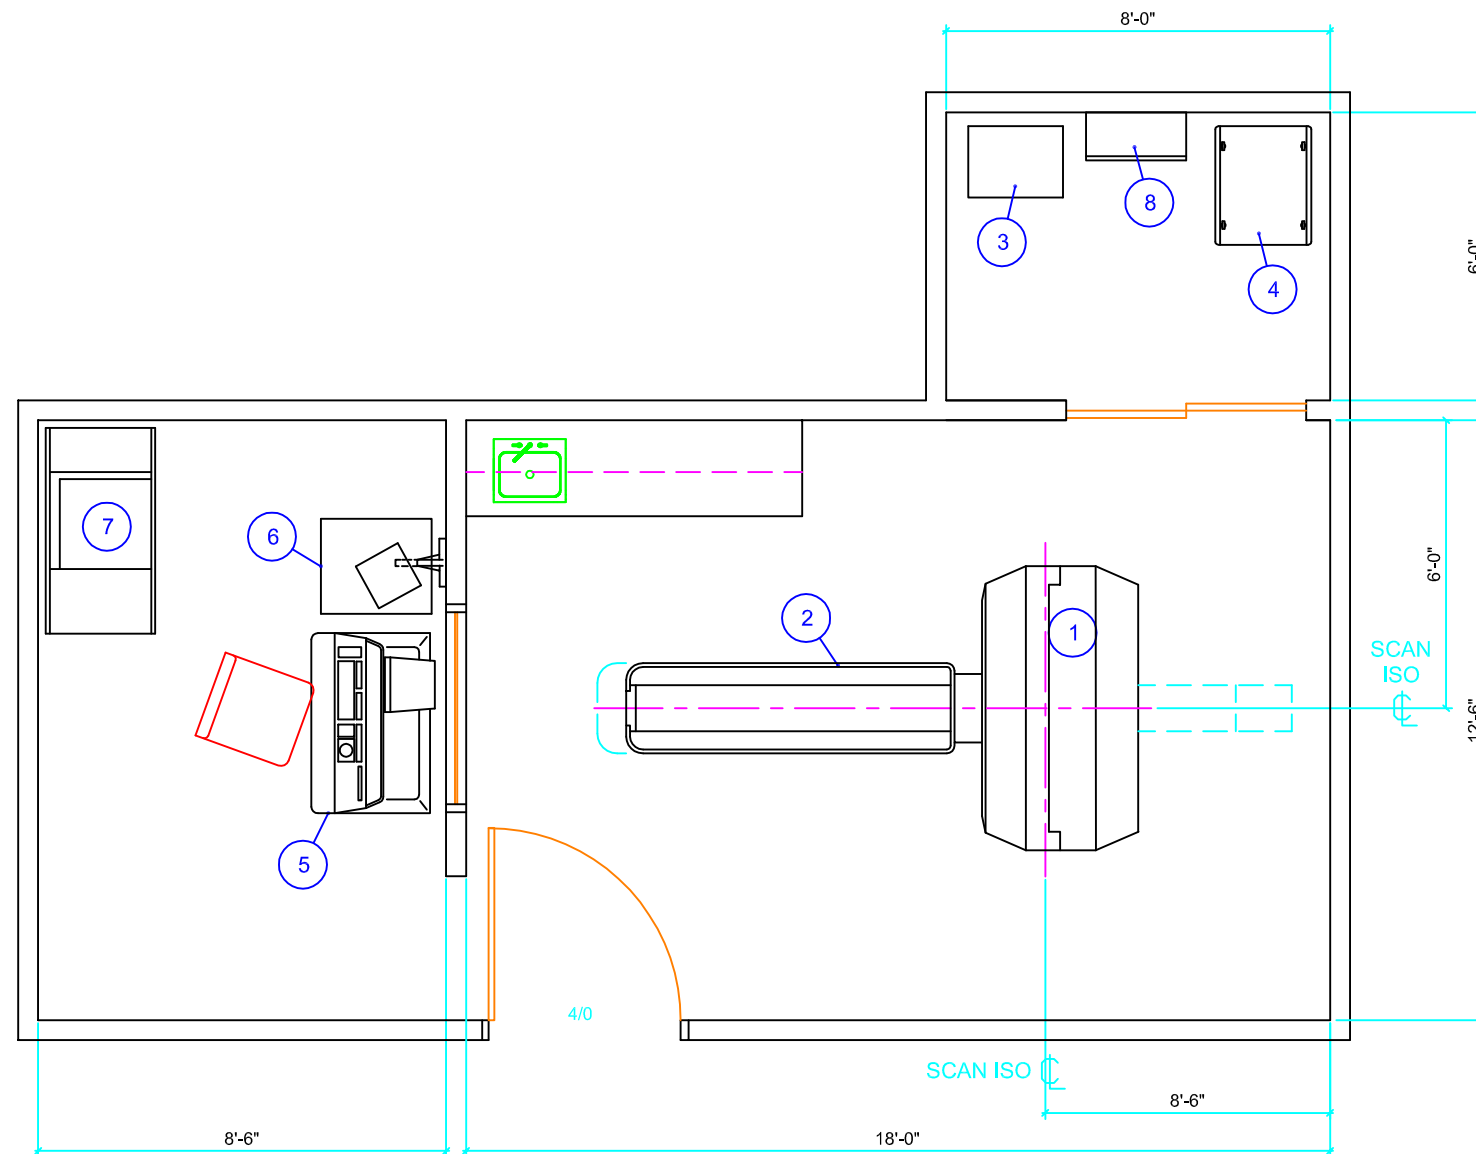

**TYPICAL ROOM AND EQUIPMENT LAYOUT**  
(DASHED LINES DEPICT EQUIPMENT TRAVEL AND SERVICE CLEARANCES)  
RECOMMENDED FINISHED CEILING HEIGHT = 8'-0"

### GENERAL NOTES

- ALL SPECIFICATIONS AND SPACE REQUIREMENTS ARE SHOWN GENERICALLY. CONTACT GAMMA TECH, INC. FOR SPECIFIC REQUIREMENTS PERTAINING TO OPTIONAL EQUIPMENT COMPONENTS AND ADDITIONAL ROOM PREPARATION SPECIFICATIONS.
- RECOMMENDED FINISHED CEILING HEIGHT IS 8'-0".  
MINIMUM FINISHED CEILING HEIGHT 7'-6".
- AMBIENT OPERATION TEMPERATURE: 71° TO 82° F.  
HUMIDITY: 20% TO 80% (NON-CONDENSING).  
ALLOWABLE TEMPERATURE CHANGE: 5°F PER HOUR  
ALLOWABLE HUMIDITY CHANGE: 5% PER HOUR  
MAX - ALTITUDE: 10,000 FT ABOVE SEA LEVEL

© PLANNING DIVISION

FILE NAME:  
GE PACE

REVISION DATE:  
01.22.2008

### POWER DEMAND

COMPONENT	MAX DEMAND (KVA)	VOLTAGE (NOM.)	CURRENT (AMP)		PHASE	REGULATION
			MOMENTARY	LONG TIME		
PWR. DIST. UNIT	50	208	139	40	3	5

## EQUIPMENT SCHEDULE

### EQUIPMENT IDENTIFICATION NUMBER

ID	DESCRIPTION	BTU / HOUR		WEIGHT (LBS.)	
		DESCRIPTION		DIMENSIONS (IN.)	
		W	D	x	H
1	GE MEDICAL SYSTEMS CT PACE GANTRY				1716
2	GE MEDICAL SYSTEMS PATIENT TABLE				539
3	GE MEDICAL SYSTEMS TABLE/GANTRY DRIVE BOX				110
4	GE MEDICAL SYSTEMS X-RAY GENERATOR				755
5	GE MEDICAL SYSTEMS OPERATORS CONSOLE				506
6	GE MEDICAL SYSTEMS MAGNETIC TAPE DRIVE				242
7	GE MEDICAL SYSTEMS LASER IMAGER SYSTEM				686
8	PowerTECH SUPPRESSOR/FILTER, WALL MOUNTED				168

PLANNING BY:



**GAMMA TECH, INC**

129 Wild Berry Lane  
Hampstead, NC 28443  
Ph (910) 270-9787 • Fax (910) 270-9767  
www.gammatech.net

