




# GE Medical Systems

## GE SYTEC 1800I CT SCANNER

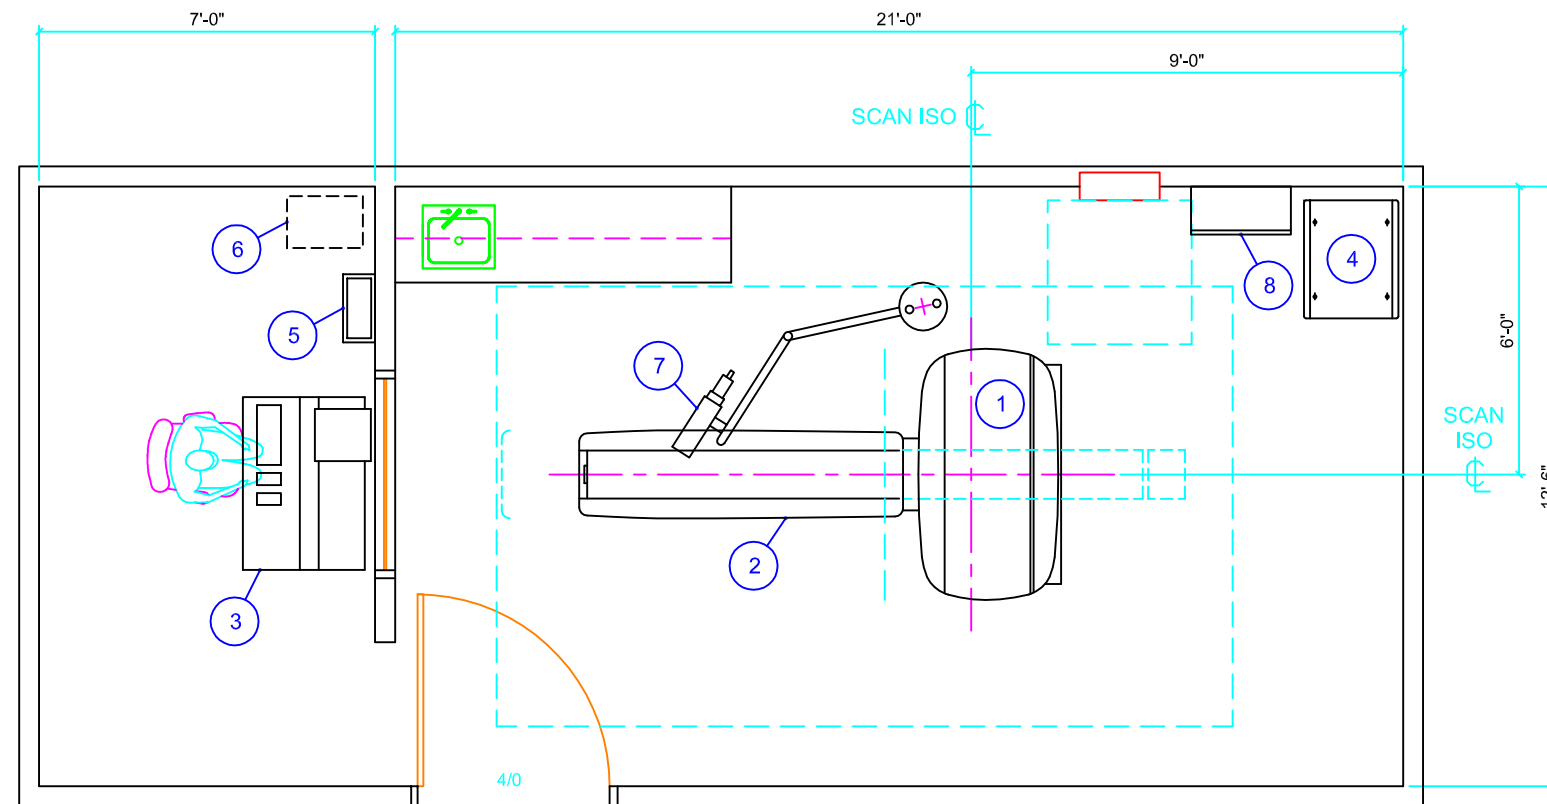

**TYPICAL ROOM AND EQUIPMENT LAYOUT**  
(DASHED LINES DEPICT EQUIPMENT TRAVEL AND SERVICE CLEARANCES)  
RECOMMENDED FINISHED CEILING HEIGHT = 8'-0"

### GENERAL NOTES

- ALL SPECIFICATIONS AND SPACE REQUIREMENTS ARE SHOWN GENERICALLY. CONTACT GAMMA TECH, INC. FOR SPECIFIC REQUIREMENTS PERTAINING TO OPTIONAL EQUIPMENT COMPONENTS AND ADDITIONAL ROOM PREPARATION SPECIFICATIONS.
- RECOMMENDED FINISHED CEILING HEIGHT IS 8'-0". MINIMUM FINISHED CEILING HEIGHT 7'-6".
- AMBIENT OPERATION TEMPERATURE: 60° TO 75° F. HUMIDITY: 30% TO 60% (NON-CONDENSING). ALLOWABLE TEMPERATURE CHANGE: 5°F PER HOUR. ALLOWABLE HUMIDITY CHANGE: 10% PER HOUR. MAX - ALTITUDE: 10,000FT ABOVE SEA LEVEL

© PLANNING DIVISION

FILE NAME:  
GE SYTEC 1800I

REVISION DATE:  
01.23.2008

## EQUIPMENT SCHEDULE

### EQUIPMENT IDENTIFICATION NUMBER

		BTU / HOUR	WEIGHT (LBS.)	
			DESCRIPTION	DIMENSIONS (IN.) W x D x H
1	5959		GE MEDICAL SYSTEMS CT SYTEC 1800I GANTRY	1210
2	397		GE MEDICAL SYSTEMS SYTEC PATIENT TABLE	948
3	1985		GE MEDICAL SYSTEMS OPERATOR'S CONSOLE	220
4	794		GE MEDICAL SYSTEMS POWER DISTRIBUTION UNIT (MUST BE LOCATED A MIN. OF 6'-0" GANTRY AND/OR CONSOLE)	755
5	1190		GE MEDICAL SYSTEMS REMOTE CONTROL FOR INJECTOR	4
6	321		GE MEDICAL SYSTEMS INJECTOR ELECTRONICS	37
7			GE MEDICAL SYSTEMS INJECTOR HEAD ON OVERHEAD COUNTERPOISED SUSPENSION	79
8			POWERTECH SUPPRESSOR/FILTER	

PLANNING BY:



**GAMMA TECH, INC**

129 Wild Berry Lane  
Hampstead, NC 28443  
Ph (910) 270-9787 • Fax (910) 270-9767  
www.gammatech.net

