




GE Medical Systems

GE SYTEC 2/3/4000 CT SCANNER

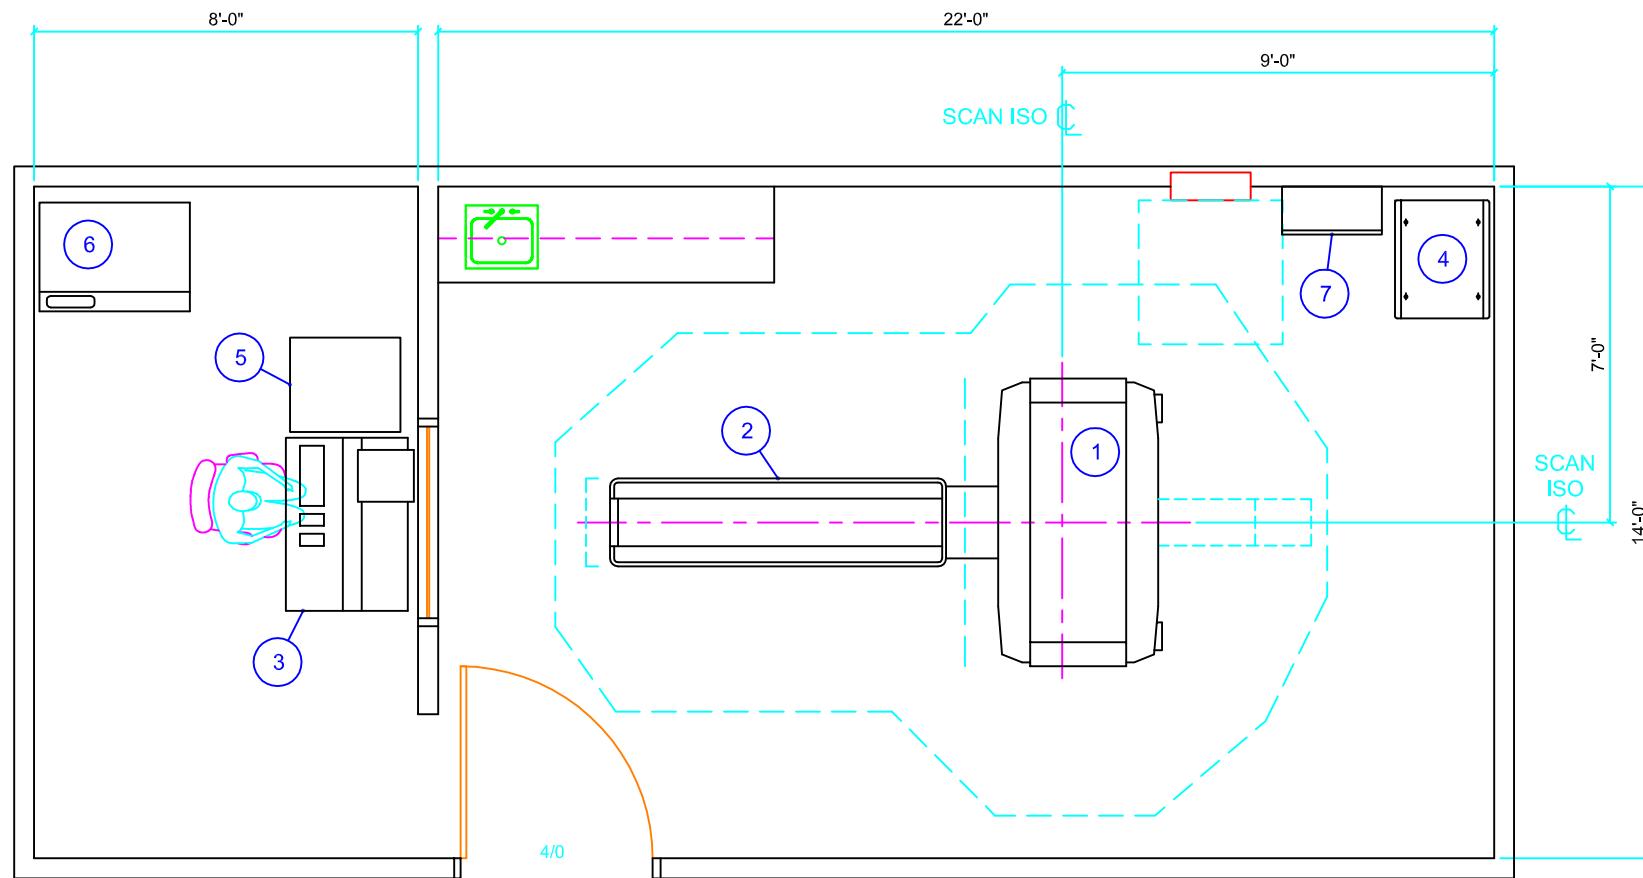

TYPICAL ROOM AND EQUIPMENT LAYOUT
(DASHED LINES DEPICT EQUIPMENT TRAVEL AND SERVICE CLEARANCES)
RECOMMENDED FINISHED CEILING HEIGHT = 8'-0"

GENERAL NOTES

- ALL SPECIFICATIONS AND SPACE REQUIREMENTS ARE SHOWN GENERICALLY. CONTACT GAMMA TECH, INC. FOR SPECIFIC REQUIREMENTS PERTAINING TO OPTIONAL EQUIPMENT COMPONENTS AND ADDITIONAL ROOM PREPARATION SPECIFICATIONS.
- RECOMMENDED FINISHED CEILING HEIGHT IS 8'-0". MINIMUM FINISHED CEILING HEIGHT 7'-6".
- AMBIENT OPERATION TEMPERATURE: 60° TO 75° F. HUMIDITY: 30% TO 60% (NON-CONDENSING). ALLOWABLE TEMPERATURE CHANGE: 5°F PER HOUR. ALLOWABLE HUMIDITY CHANGE: 10% PER HOUR. MAX - ALTITUDE: 10,000FT ABOVE SEA LEVEL.

© PLANNING DIVISION

FILE NAME:
GE SYTEC 2_3_4000

REVISION DATE:
01.23.2008

EQUIPMENT SCHEDULE

EQUIPMENT IDENTIFICATION NUMBER

		BTU / HOUR	WEIGHT (LBS.)	
			DESCRIPTION	DIMENSIONS (IN.) W x D x H
1	5955		GE MEDICAL SYSTEMS CT SYTEC 2/3/4000 GANTRY	1716
2			GE MEDICAL SYSTEMS PATIENT TABLE W/ EXTENDED TABLE	800
3	5956		GE MEDICAL SYSTEMS 2/3/4000 OPERATOR'S CONSOLE	507
4	794		GE MEDICAL SYSTEMS X-RAY GENERATOR (MUST BE LOCATED A MIN. OF 6'-0" GANTRY AND/OR CONSOLE)	755
5	1190		GE MEDICAL SYSTEMS MAGNETIC TAPE DRIVE UNIT	242
6	2520		GE MEDICAL SYSTEMS 969 LASER IMAGER SYSTEM	610
7	300		PowerTECH SUPPRESSOR/FILTER WALL MOUNTED	168

PLANNING BY:



GAMMA TECH, INC

129 Wild Berry Lane
Hampstead, NC 28443
Ph (910) 270-9787 • Fax (910) 270-9767
www.gammatech.net

