




GE Medical Systems

GE SYTEC 6000/8000 CT SCANNER

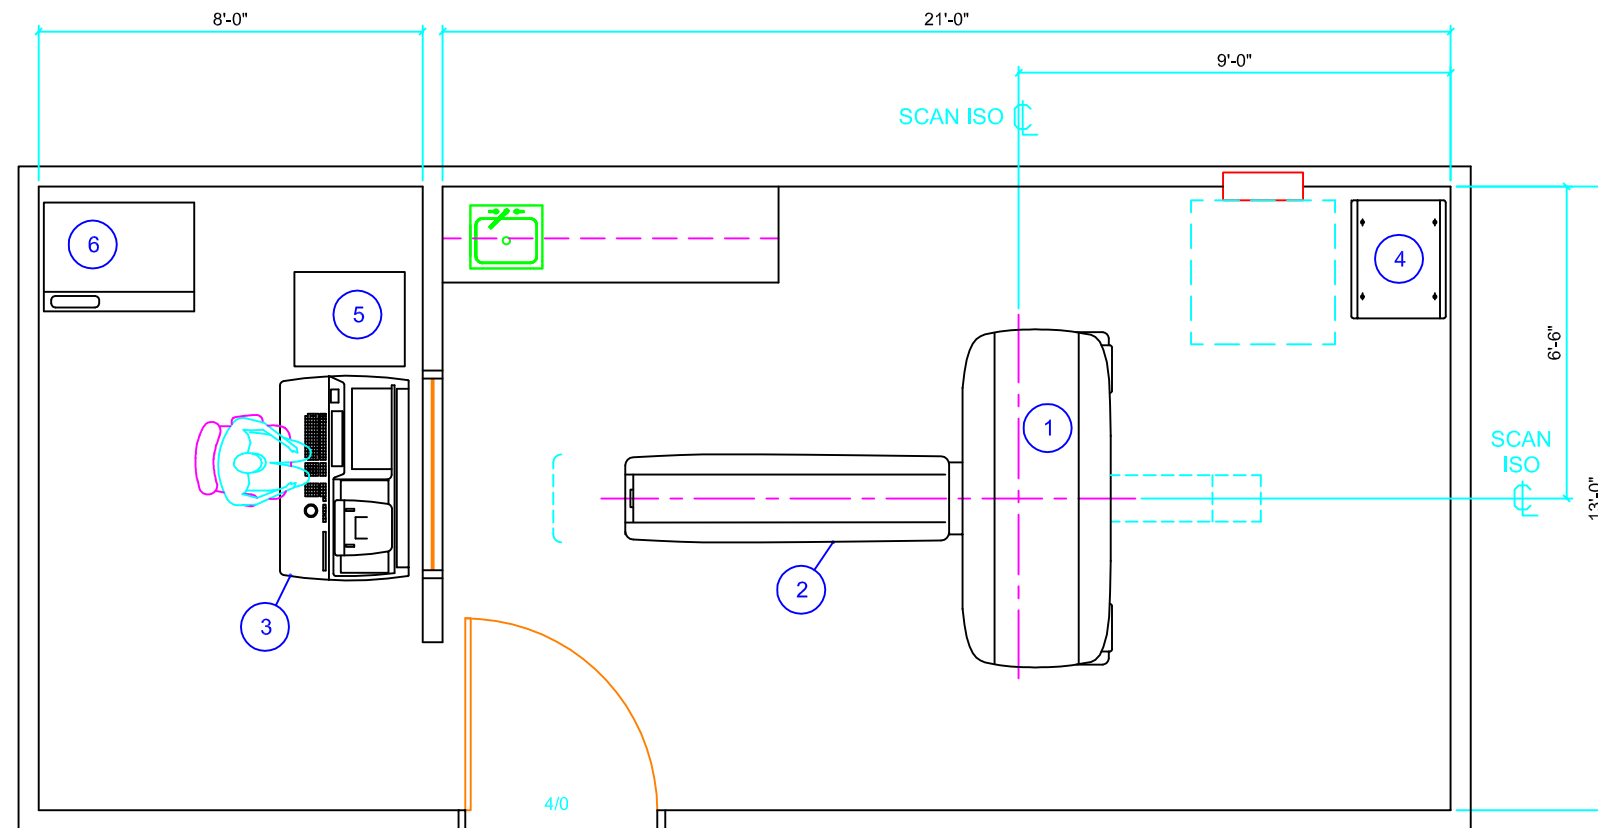

TYPICAL ROOM AND EQUIPMENT LAYOUT
(DASHED LINES DEPICT EQUIPMENT TRAVEL AND SERVICE CLEARANCES)
RECOMMENDED FINISHED CEILING HEIGHT = 8'-0"



GENERAL NOTES

- ALL SPECIFICATIONS AND SPACE REQUIREMENTS ARE SHOWN GENERICALLY. CONTACT GAMMA TECH, INC. FOR SPECIFIC REQUIREMENTS PERTAINING TO OPTIONAL EQUIPMENT COMPONENTS AND ADDITIONAL ROOM PREPARATION SPECIFICATIONS.
- RECOMMENDED FINISHED CEILING HEIGHT IS 8'-0". MINIMUM FINISHED CEILING HEIGHT 7'-6".
- AMBIENT OPERATION TEMPERATURE: 68° TO 82° F. HUMIDITY: 40% TO 80% (NON-CONDENSING).
MAX - ALTITUDE: 8,000FT ABOVE SEA LEVEL

© PLANNING DIVISION

FILE NAME:
GE SYTEC 6000/8000

REVISION DATE:
01.23.2008

EQUIPMENT SCHEDULE

EQUIPMENT IDENTIFICATION NUMBER

		BTU / HOUR	DESCRIPTION	WEIGHT (LBS.)	
				DIMENSIONS (IN.) W x D x H	
1	11116		GE MEDICAL SYSTEMS CT SYTEC 6000/8000 GANTRY		2535
2	397		GE MEDICAL SYSTEMS SYTEC PATIENT TABLE		948
3	5995		GE MEDICAL SYSTEMS OPERATOR'S CONSOLE		507
4	3176		GE MEDICAL SYSTEMS POWER DISTRIBUTION UNIT (MUST BE LOCATED A MIN. OF 6'-0" GANTRY AND/OR CONSOLE)		755
5	1190		GE MEDICAL SYSTEMS MAGNETIC TAPE DRIVE		242
6	2520		GE MEDICAL SYSTEMS 969 LASER IMAGER SYSTEM		242

PLANNING BY:



GAMMA TECH, INC

129 Wild Berry Lane
Hampstead, NC 28443
Ph (910) 270-9787 • Fax (910) 270-9767
www.gammatech.net