



**Philips Medical Systems**  
**MEDIO 50 CP / BT-S4**  
**RAD./TOMO. SUITE**

**GENERAL NOTES**


• ALL SPECIFICATIONS AND SPACE REQUIREMENTS ARE SHOWN GENERICALLY. CONTACT GAMMA TECH, INC. FOR SPECIFIC REQUIREMENTS PERTAINING TO OPTIONAL EQUIPMENT COMPONENTS AND ADDITIONAL ROOM PREPARATION SPECIFICATIONS.

© PLANNING DIVISION  
 FILE NAME:  
 PHILIPS MEDIO 50 CP  
 RAD/TOMO SYSTEM  
 REVISION DATE: 01/08/2010


**EQUIPMENT SCHEDULE**

**EQUIPMENT IDENTIFICATION NUMBER**

	BTU / HOUR	DESCRIPTION	WEIGHT (LBS.)			
			DIMENSIONS (IN.)			
			W	x	D	x
1	171	PHILIPS MEDICAL SYSTEMS MEDIO 50 CP CONTROL DESK (COUNTER MOUNTED)	19.50	16.88	6.63	27
2	1368	PHILIPS MEDICAL SYSTEMS MEDIO 50 CP GENERATOR	39.12	23.50	29.50	551
3	1000	PHILIPS MEDICAL SYSTEMS BT-S4 RAD/TOMO TABLE	94.49	43.31	44.88	
4	760	PHILIPS MEDICAL SYSTEMS CS-62BT OVER HEAD TUBE CRANE	157.50	92.75	105.00	594
5	400	PHILIPS MEDICAL SYSTEMS VERTICAL DIAGNOST 1 TILTING BUCKY STAND	26.50	39.38	81.50	332

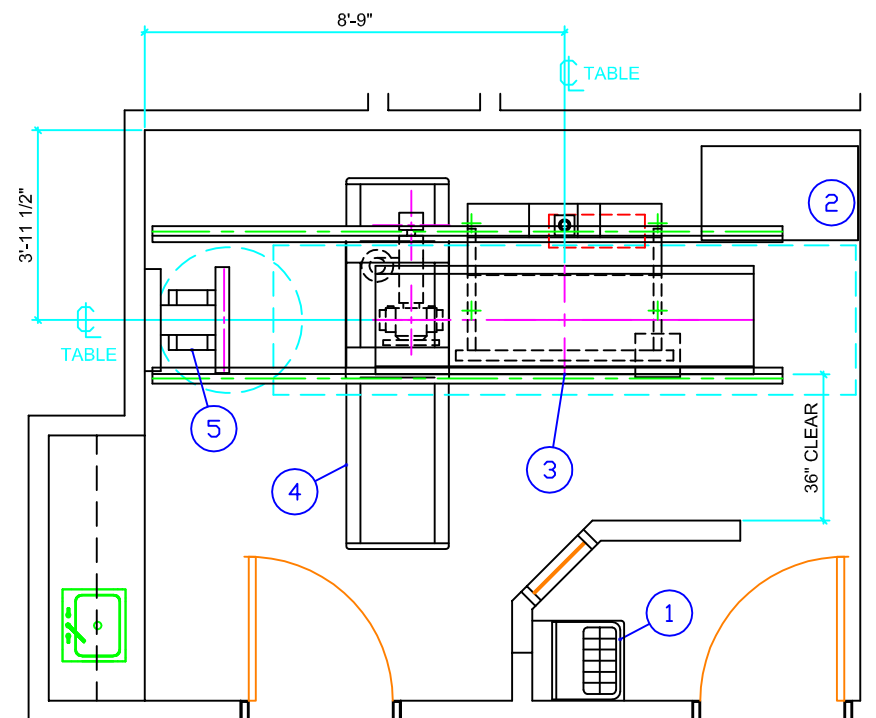

TYPICAL ROOM AND EQUIPMENT LAYOUT



PLANNING BY:



**GAMMA TECH, INC**

129 Wild Berry Lane  
 Hampstead, NC 28443  
 Ph (910) 270-9787 • Fax (910) 270-9767  
 www.gammatech.net