

**GENERAL NOTES**


- ALL SPECIFICATIONS AND SPACE REQUIREMENTS ARE SHOWN GENERICALLY. CONTACT GAMMA TECH, INC. FOR SPECIFIC REQUIREMENTS PERTAINING TO OPTIONAL EQUIPMENT COMPONENTS AND ADDITIONAL ROOM PREPARATION SPECIFICATIONS.
- RECOMMENDED CEILING HEIGHT IS 9'-0".
- SUGGESTED AMBIENT ROOM REQUIREMENTS ARE 66° - 75° F AT 30% TO 60% R.H. (NON-CONDENSING).
- INCOMING POWER SUPPLIES:  
MAIN: VARIES WITH GENERATOR KW RATING.  
AUXILLARY: 208/120VAC, 60AMP DISCONNECT.

© PLANNING DIVISION  
FILE NAME:  
QG\_QT750\_RS-580.DWG  
REVISION DATE: 01/08/2010


**EQUIPMENT SCHEDULE**

NOTES	EQUIPMENT IDENTIFICATION NUMBER	BTU / HOUR	WEIGHT (LBS.)				
			DESCRIPTION	DIMENSIONS (IN.)			
				W	x	D	x
OFOI	1	130	QUANTUM ODYSSEY QG -SERIES GENERATOR CONTROL CONSOLE	17.90	12.25	3.31	5
OFOI	2	3600	QUANTUM ODYSSEY QG -SERIES GENERATOR RACK CABINET	24.00	20.00	33.50	380
OFOI	3	400	QUANTUM QT-750 ELEVATING FLOAT TOP TABLE	85.00	35.55	32.50	500
OFOI	4	1200	QUANTUM RS-580 CTM CEILING MOUNTED TUBE SUPPORT	168.00	118.50	112.79	1200
OFOI	5	35	QUANTUM QW-420 VERTICAL WALL STAND	26.00	14.50	84.00	225
OFOI	6	35	QUANTUM OPTIONAL QG-HSS (Q OR R STATOR) HIGH SPEED STARTER (WALL MOUNT)	19.00	12.00	5.00	40

NOTE EXPLANATION:  
CFCI = CONTRACTOR FURNISHED - CONTRACTOR INSTALLED  
OFCI = OWNER FURNISHED - CONTRACTOR INSTALLED  
OFOI = OWNER FURNISHED - OWNER INSTALLED

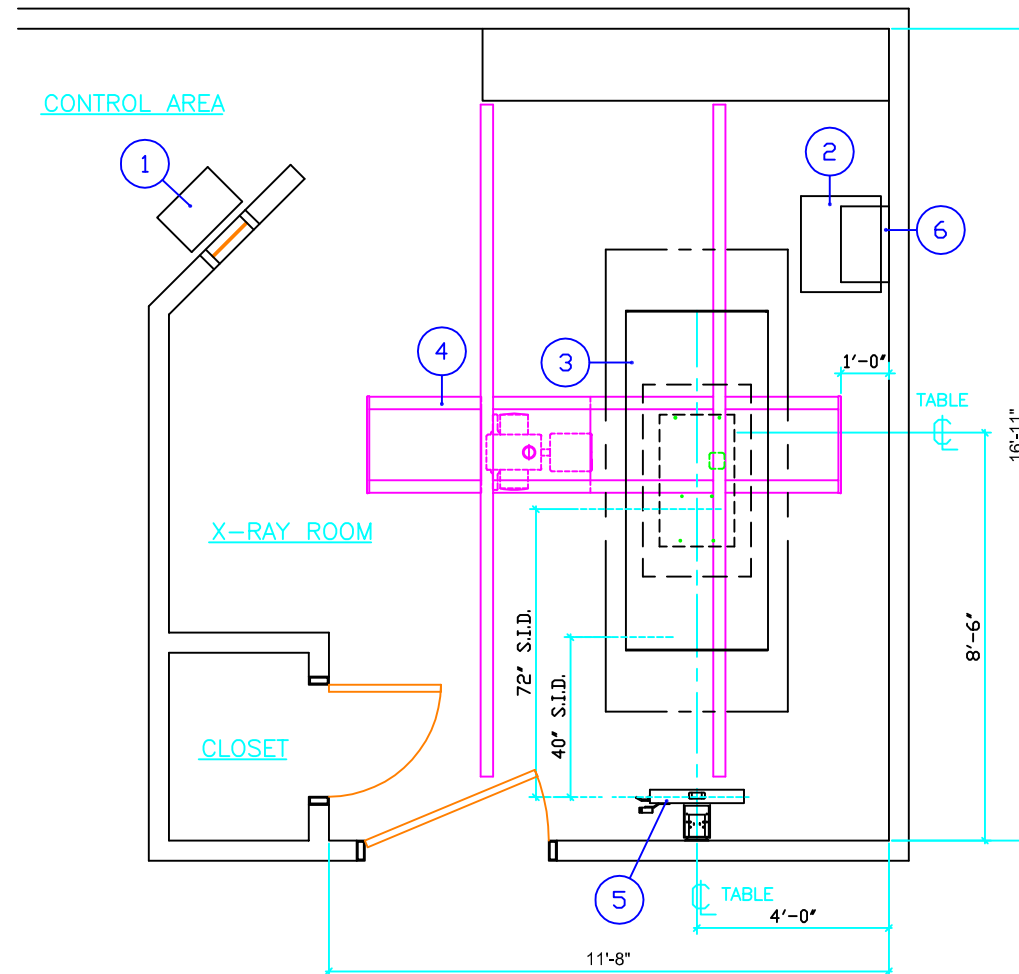

TYPICAL ROOM LAYOUT



PLANNING BY:



**GAMMA TECH, INC**

129 Wild Berry Lane  
Hampstead, NC 28443  
Ph (910) 270-9787 • Fax (910) 270-9767  
www.gammatech.net