


# TYPICAL ROOM LAYOUT

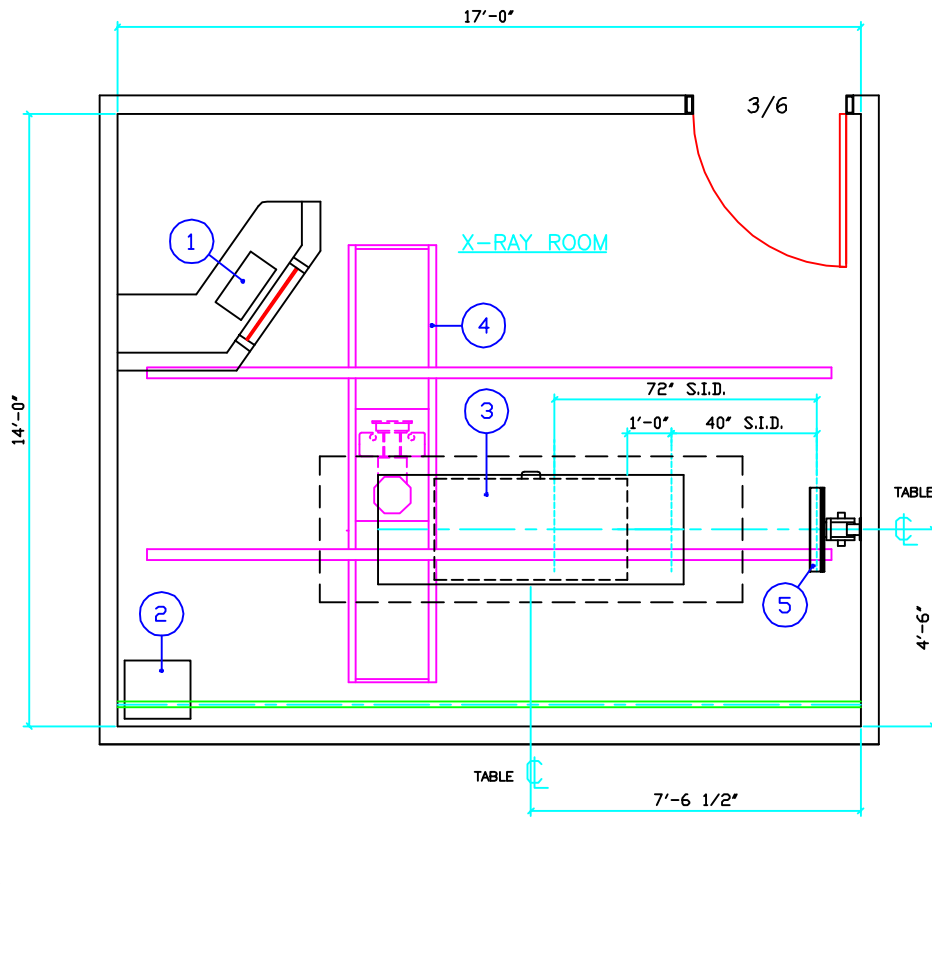

## GENERAL NOTES

- ALL SPECIFICATIONS AND SPACE REQUIREMENTS ARE SHOWN GENERICALLY. CONTACT GAMMA TECHNOLOGIES FOR SPECIFIC REQUIREMENTS PERTAINING TO OPTIONAL EQUIPMENT COMPONENTS AND ADDITIONAL ROOM PREPARATION SPECIFICATIONS.
- RECOMMENDED CEILING HEIGHT IS 8'-6".
- SUGGESTED AMBIENT ROOM REQUIREMENTS ARE 66° TO 75° F. AT 30% TO 60% R.M. (NON-CONDENSING).
- MAIN INCOMING POWER SUPPLY: VARIES WITH GENERATOR MODEL.

## EQUIPMENT SCHEDULE

		EQUIPMENT IDENTIFICATION NUMBER				
		BTU / HOUR	WEIGHT (LBS.)			
		DESCRIPTION	DIMENSIONS (IN.) W x D x H			
1	25	SUMMIT SYNERGY 200KHZ GENERATOR OPERATOR CONTROL PANEL	17.00	8.50	3.00	4
2	544	SUMMIT SYNERGY 200KHZ GENERATOR POWER CABINET	18.00	16.00	37.00	245
3	35	SUMMIT MODEL S-211 ELEVATING FOUR WAY FLOAT TOP TABLE	84.00	30.00	34.00	640
4	1200	SUMMIT GX-CTM (3310) CEILING SUSPENDED X-RAY TUBE CRANE	188.00	108.00	102.00	600
5	35	SUMMIT MODEL S-109 VERTICAL BUCKY STAND	24.00	14.00	86.00	183
6						
7						
8						

## SUMMIT HIGH FREQUENCY RADIOGRAPHIC SYSTEM SUITE.

**GAMMA TECH, INC**



129 Wild Berry Lane  
Hampstead, NC 28443  
Ph (910) 270-9787  
Fax (910) 270-9767  
www.gammatech.net

© PLANNING DIV.

FILE NAME:  
SYN200\_3310\_211

REVISION DATE:  
01.05.2012  
D.J. HENRY